



Agustinus Purna Irawan <agustinus@untar.ac.id>

Manuscript for IJET

1 message

Agustinus Purna Irawan <agustinus@untar.ac.id>
To: editorijet@enggjournals.com

Mon, Apr 11, 2016 at 11:20 AM

Dear IJET Managing Editor

International Journal of Engineering and Technology

Herewith, we submit a manuscript for IJET:

Title: Mechanical Characteristics of Rattan Reinforced Fiberglass and Epoxy Composites for Shank Prosthesis Application.

Authors: Agustinus Purna Irawan, Frans Jusuf Daywin, Fanando, Tommy Agustino

Institution: Mechanical Engineering Department, Faculty of Engineering, Tarumanagara University, Jakarta, Indonesia.

We hope that our manuscript can be published in IJET. Thank you very much for your attention and collaboration.

Best Regards,

Agustinus Purna Irawan

Prof. Dr. Agustinus Purna Irawan
Professor of Mechanical Engineering

Dean of Faculty of Engineering
Tarumanagara University
Jakarta - Indonesia
Phone : +62215663124
Fax : +62215663277

Mobile : +628129672348
www.tarumanagara.ac.id

2 attachments

 **Agustinus Purna Irawan et al-UNTAR-IJET-April 2016.doc**
9547K

 **Copyright Transfer-IJET-Agustinus Purna Irawan et al-10 April 2016.pdf**
371K



Agustinus Purna Irawan <agustinus@untar.ac.id>

Manuscript Submission Confirmation of IJET Re: Manuscript for IJET

2 messages

Editor IJET <editorijet@enggjournals.com>
To: agustinus@untar.ac.id

Mon, Apr 11, 2016 at 11:20 AM

Dear Author,

Read the author guidelines at <http://www.enggjournals.com/ijet/author-guidelines.html> and send the paper. If you have already sent the copyright form duly signed by all authors then ignore this email. If you haven't send us the scanned copy of the copyright form of all the authors duly signed by pen, send it immediately with the manuscript once again. We don't accept signature images inserted in the copyright form. Send us the copyright form individually signed by authors. Then only we will send it to review your manuscript else we don't consider it. Send the manuscript and copyright form to editorijet@enggjournals.com. You can download the copyright from from <http://www.enggjournals.com/ijet/docs/IJETCopyrightAgreement.pdf>. You will get manuscript id within two days if you have sent all required documents to us. If you didn't get any acknowledgement from us then resend the paper with all documents. Check your spam folder before sending email to us.

Regards,
Editor,
IJET.

Website : <http://www.enggjournals.com/ijet/>
e-ISSN : 0975-4024
p-ISSN : 2319-8613

Agustinus Purna Irawan <agustinus@untar.ac.id>
To: Editor IJET <editorijet@enggjournals.com>

Tue, Apr 12, 2016 at 8:21 AM

Dear Managing Editor
International Journal Engineering and Technology

Thank you for your reply to our email. Refer your email, herewith, we send once again our manuscript and scanned copy of the copyright form of all authors duly signed by pen.
Thank you very much for your attention and collaboration.

Best Regards,

Agustinus Purna Irawan

Prof. Dr. Agustinus Purna Irawan
Professor of Mechanical Engineering

Dean of Faculty of Engineering
Tarumanagara University
Jakarta - Indonesia
Phone : +62215663124
Fax : +62215663277
Mobile : +628129672348
www.tarumanagara.ac.id
[Quoted text hidden]

2 attachments

Agustinus Purna Irawan et al-UNTAR-IJET-12 April 2016.doc
9547K

Copyright Transfer-IJET-Agustinus Purna Irawan et al-12 April 2016.pdf
470K



Agustinus Purna Irawan <agustinus@untar.ac.id>

Manuscript Outcome of IJET16-08-03-050

3 messages

IJET Editor <ijet@enggjournals.com>
To: agustinus@untar.ac.id

Mon, Jun 20, 2016 at 6:12 PM

Dear Author,

Your manuscript id is IJET16-08-03-050. Please use this manuscript id in future communication.

Your Manuscript entitled " Mechanical Characteristics of Rattan Reinforced Fiberglass and Epoxy Composites for Shank Prosthesis Application " has been accepted for publication. Please pay the manuscript handling charges within 3 days to publish your paper. Send us your manuscript in word document format to process further with the below corrections. If the below corrections are not performed we don't publish the manuscript.

1. The format of the paper is not in IJET Template.
2. Some images are not clear. Change the images in the paper to high quality images.
3. Equations should be in Equation Editor. Don't send equations in image format or print screen format.
4. Tables should be in text format, and tables should not be in figures and not print screen format.
5. If you had taken any part/figure/table from any other research paper then kindly mention it in references.

Kindly send back the scanned copy of the manuscript handling charges remittance pay in slip for sum of US\$300/- If you want hard copy of the journal pay additional US\$100.

NOTE: All The Transaction Charges Or Service Charges Should be paid by the Author Only. (Like Inter Banking Charges, NEFT Charges, Wire Transfer Charges etc.)

We don't accept DD or Cheque payment.

If you got acceptance from more than 1 paper you can combine the total amount and can do a single payment instead of doing individual payment.

If you haven't sent us the copyright form please send it asap. Send us the manuscript in IEEE format as we have mentioned in our website in word document.

You can download the template from http://www.enggjournals.com/ijet/docs/IJET_Paper_Word_Template_A4_V5.doc

You can download the copyright form from <http://www.enggjournals.com/ijet/docs/IJETCopyrightAgreement.pdf>

Account Holder Name	:	ENGG JOURNALS PUBLICATIONS
Bank Name	:	HDFC Bank
Branch Name	:	Perungalathur, Chennai
Account Number	:	50200008830311
Swift Code	:	HDFCINBBCHE
IBAN	:	HDFCINBB
IFSC Code/Routing No.	:	HDFC0001871
Bank Address	:	16/24, Srinivasa Raghavan Road, New Perungalathur, Chennai - 600063, Tamil Nadu

Please reply along with the above mentioned particulars within two days.

If you wish to pay by credit card through Paypal, Payza or Liberty Reserve let us know we will send you the link to do payment. There is an additional charge of 6% if you pay by Paypal, Payza or Liberty Reserve.

Thanks & Regards,

Editor-in-Chief,

IJET.

website : <http://www.enggjournals.com/ijet/>

e-ISSN : 0975-4024

p-ISSN : 2319-8613

Agustinus Purna Irawan <agustinus@untar.ac.id>
To: IJET Editor <ijet@enggjournals.com>

Wed, Jun 22, 2016 at 1:46 PM

Dear Editor in Chief of IJET,

I herewith submit the revised manuscript id is IJET16-08-03-050 in accordance with the correction that was sent, and the copyright transfer form.

I send also a scanned of the manuscript handling charges remittance pay-in slip for the sum of US \$ 300 / -

Thank you very much for your attention and cooperation.

Best Regards,
agustinus

Prof. Dr. Agustinus Purna Irawan
Professor of Mechanical Engineering

Dean of Faculty of Engineering
Tarumanagara University

Jakarta - Indonesia

Phone : +62215663124

Fax : +62215663277

Mobile : +628129672348

www.tarumanagara.ac.id

[Quoted text hidden]

3 attachments

 **Agustinus Purna Irawan et al-UNTAR-IJET 16-08-03-050.doc**
9548K

 **Copyright Transfer-IJET-Agustinus Purna Irawan et al-IJET 16-08-03-050.pdf**
470K

 **Scanned of the manuscript handling charges-IJET 16-08-03-050.pdf**
941K

IJET Editor <ijet@enggjournals.com>
To: Agustinus Purna Irawan <agustinus@untar.ac.id>

Mon, Jun 27, 2016 at 1:24 PM

Dear Author,

We have received your payment successfully. We will send you the Gallery Proof within 7 days.

If you haven't sent us the manuscript in the format as we have mentioned in our website in the word document, send it immediately.

If you haven't sent us the scanned copy of the copyright form of all the authors send it to us asap. We need the copyright form from all authors. If you have ordered Hard Copy from us, Send us the address for communication with postal code and phone number to send you the hard copy. Your manuscript will be published online on 30-June-2016.

Regards,
Editor-in-Chief,
IJET.

Website : <http://www.enggjournals.com/ijet/>
e-ISSN : 0975-4024
p-ISSN : 2319-8613

**Agustinus Purna Irawan <agustinus@untar.ac.id>**

Gallery Proof of IJET16-08-03-050

2 messages

IJET Acceptance <ijetacceptance@enggjournals.com>

Mon, Jun 27, 2016 at 6:30 PM

Reply-To: ijet@enggjournals.comTo: agustinus@untar.ac.id

Dear Author,

With this I am attaching the Gallery Proof. Let us know if there are any corrections within 2 days. We will send you the word document to do the corrections.

Regards,
Editor,
IJET.

 IJET16-08-03-050.pdf

983K

Agustinus Purna Irawan <agustinus@untar.ac.id>

Tue, Jun 28, 2016 at 12:03 PM

To: Siva IJET <ijet@enggjournals.com>

Dear Editor of IJET,

Thank you very much for your information. The final manuscript is ok.

best regards,

agustinus

**Prof. Dr. Agustinus Purna Irawan
Professor of Mechanical Engineering**

Dean of Faculty of Engineering

Tarumanagara University

Jakarta - Indonesia

Phone : +62215663124

Fax : +62215663277

Mobile : +628129672348

www.tarumanagara.ac.id

[Quoted text hidden]

Mechanical Characteristics of Rattan Reinforced Fiberglass and Epoxy Composites for Shank Prostheses Application

Agustinus Purna Irawan ^{#1}, Frans Jusuf Daywin ^{#2}, Fanando ^{#3}, Tommy Agustino ^{#4}

^{#1,2,3,4} Mechanical Engineering Department, Faculty of Engineering, Tarumanagara University
Jl. Letjen. S. Parman No. 1 Jakarta, Indonesia 11440

¹ agustinus@untar.ac.id

Abstract—This research aims to develop a rattan laminated fiberglass epoxy resin materials (RLFERM) to increase of mechanical strength especially in tensile, compressive, impact and flexural strength. The RLFERM will be used as an alternative material for shank prosthesis endoskeletal type and another use in engineering design. This research is related to the utilization of the natural potential of Indonesia especially of rattan. The method used to produce the endoskeletal material by using laminated process of rattan with fiberglass and epoxy resin. The test conducted involves the tensile, compressive, impact and flexural strength. The result showed that there was an increase in strength of RLFERM compared with rattan without lamination (Natural Rattan, NR). Tensile strength of RLFERM (80.2 MPa) and $E = 8.6$ GPa increased by 67.8% when compared to the tensile strength of NR (47.8 MPa) and $E = 6.4$ GPa. Compressive strength of RLFERM increased 47.2%, from 31.8 MPa to 46.8 MPa, impact strength of RLFERM increased 64%, from 39 kJ/m² to 64 kJ/m², and flexural strength of RLFERM increased on average by 53% from 54.1 MPa to 82.3 MPa. Increasing strength of RLFERM is obtained from good interface between surface of rattan with fiberglass and epoxy resin as laminate. The first prototype of lower limb prosthesis with a shank prosthesis endoskeletal type of RLFERM, have been made with good results and tested for use by patient. The test results indicate that the lower limb prosthesis with a shank prosthesis components made from RLFERM can be used by patients to walk properly and has good strength. This result will be a reference for further research in the development of a shank prosthesis made from rattan and another use in engineering design.

Keyword-Rattan, Laminated, Mechanical strength, Shank, Endoskeletal type

I. INTRODUCTION

Indonesia have many potential of natural materials such as rattan, bamboo, wood, and natural fiber [1]-[3]. This potential has not been fully used in the design and development of manufacturing products of high added value. In this study, we have developed an alternative materials for the product of shank prosthesis (lower limb prosthesis), specifically in endoskeletal type by using rattan material.

Lower limb prosthesis is divided into above knee and below knee prosthesis, performed by amputation [4]. Research and design of lower limb prosthesis continues to grow and has gained a new invention including materials, design, installation method, gait analysis and evaluation of the performance of the prosthesis after being used in a certain period of time by the patient. Stark [5] stated that the development of modern prosthetic should consider a few things such as functions, indications, and cost. Innovation prosthetic requires more knowledge in the field of foot physiologic function and more descriptive terminology. Five things that should be considered are load bearing, leverage, shock absorption, balance, and protection [5].

Campbell [6], Faulker *et al* [7], Khazraji *et al* [8] stated that a variety of materials have been used in the development of a prosthesis, such as metals, polymers, composites, and natural materials such as wood and leather. Material selection is not only concerned with functional requirements, but also the price, manufacturing processes, availability of materials and ease of repair and maintenance [9]. Irawan *et al* [1] has developed a socket made from ramie fiber reinforced epoxy composites. Sockets made from ramie fiber reinforced epoxy composites generate good strength and comfort for the patient. Socket component is also developed by using bamboo fiber composite, rattan fiber composite and banana composite materials [2], [10], [11]. Natural materials have the potential to develop as materials for lower limb prosthetic component.

An important component of the lower limb prosthesis is shank prosthesis. Some of the materials used to make the component of the shank are aluminum, titanium, mild steel, thermosetting plastic, stainless steel, and graphite. The development of the use of natural materials that are currently carried out in various fields by considering the ability of recycling and renewable, encourages research prosthesis using natural materials [9].

Similarly, the development of a prosthesis material also leads to the use of natural materials that are environmentally friendly. Shasmin *et al* [12] has developed a tube section (shank) with use of bamboo. Based on the results of these studies, the results are obtained that the tube made of bamboo has good strength and can be applied to the design of the prosthesis especially for shank component.

This research aims to develop alternative materials to produce the shank of endoskeletal type with rattan materials. Research of rattan as a material of the shank component is a very important. This is related to the utilization of the natural potential of Indonesia especially rattan. The results of various studies have been published which show that the rattan potential to be developed as biomaterials, especially to produce shank prosthesis endoskeletal type.

II. MATERIAL AND METHOD

A. Materials

Rattan laminated fiberglass epoxy resin materials (RLFERM) is made with a layer of material from the inside to the outside as follows: rattan diameter (30-40) mm with a surface made rough with depth of (0.5-1.5) mm, as much as two-ply stockinette layer with thickness of (0.5-1) mm as the inner reinforcement is placed on the surface of rattan, a layer of fiberglass shaped fiber mat (woven) as a single layer with a thickness of (1-2) mm, three layers of stockinette layer with thickness of (0.5-1) mm as outer reinforcement, and a protective outer plastic layer by one layer. The lamination process is done by pouring a mixture of epoxy resin and hardener to resin ratio of 1:1, by casting the channel. Lamination process is followed by the press and vacuum until -50 bar. The vacuum process aims to help accelerate the lamination process and eliminate void.

B. Method

Macrostructure test of a sample of rattan is to observe the pore structure of the rattan, so it can be determined the optimum surface area of rattan in the theoretical calculations. This is necessary because the rattan is a porous material that needs to be calculated solid surface that can be used in the calculation of the surface area [13]. Theoretical calculation of rattan strength uses the equations of mechanical strength by considering the porous surface area which is obtained from macrostructure test. Strength simulation and analysis of rattan uses computer software. The results of this simulation are used for comparative data on the results of testing the strength of rattan.

Mechanical strength testing included tensile, compressive, impact and flexural strength testing of Natural Rattan (without lamination, NR) and RLFERM. Tensile strength testing aims to determine the maximum tensile strength and elasticity modulus of rattan to be used as a shank material. Tensile strength testing uses a Universal Testing Machine. Compressive strength testing aims to determine the maximum compressive of rattan to be used as a shank material. Compressive strength is required by shank prosthesis material so as to receive a compressive load of the weight and the dynamic movement of the lower limb while walking [14]. Impact strength testing aims to determine the maximum impact of rattan to be used as a shank material, especially to provide a sense of safety when it is used for walking and when it receives impact loads from other objects [14]. Flexural strength testing aims to get the maximum bending strength of rattan. Bending strength is associated with flexural strength of rattan materials that is needed on the shank material with the purpose to provide comfort for the user.

After testing the mechanical strength, we developed a prototype prosthesis shank to be tested and used by the patient. Results of testing the prototype of this first level will be a reference for the development of next prototype.

III. RESULT AND DISCUSSIONS

A. Macrostructure Test of Rattan

Rattan is a material with a porous structure [15]. In the theoretical strength calculation, rattan surface area should be calculated by considering the pore surface area, so it can produce strength such as real strength [16], [17]. To obtain the pore surface data, the test is conducted with as many as 10 samples of rattan. Fig. 1 shows the result sample test of rattan surface with 7 times magnification.

The number of pores is counted and measured to obtain the surface area porous of rattan, so the surface area of solid rattan can be calculated as a reference to calculate the strength. Based on the macrostructure test results of 10 samples, a total solid surface area of 665 mm^2 is obtained. The ratio of the surface area of the solid area and the average total surface area is 0.84 (Table I). This ratio is used as the data to calculate theoretical strength of natural rattan.

TABLE I. Ratio of Surface Area of Rattan

	Diameter r (mm)	Surface Area (mm ²)	Number of Pores	Diameter of Pores (mm ²)	Surface Area per Pores (mm ²)	Pores Area (mm ²)	Solid Area (mm ²)	Ratio
Max	32.5	829	1026	0.42	0.14	142	714	0.86
Min	29.5	683	1005	0.37	0.11	108	563	0.82
Av	32	787	1015	0.39	0.12	124	665	0.84
SD	0.88	42.81	7.44	0.01	0.01	8.91	41.57	0.01

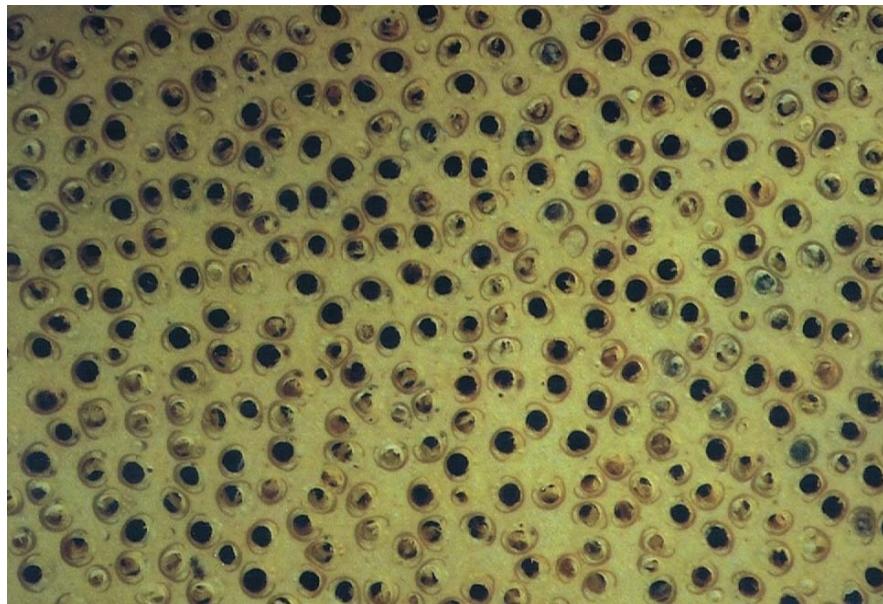


Fig. 1. Macrostructure test result

B. Tensile Strength

Fig. 2 shows an example of a RLFERM product that is produced by using lamination process with fiberglass and epoxy resin. The thickness of the outer layer of rattan with the lamination process is 3-5 mm. Lamination process produces a good interface between the surface of the rattan with fiberglass and epoxy resin.

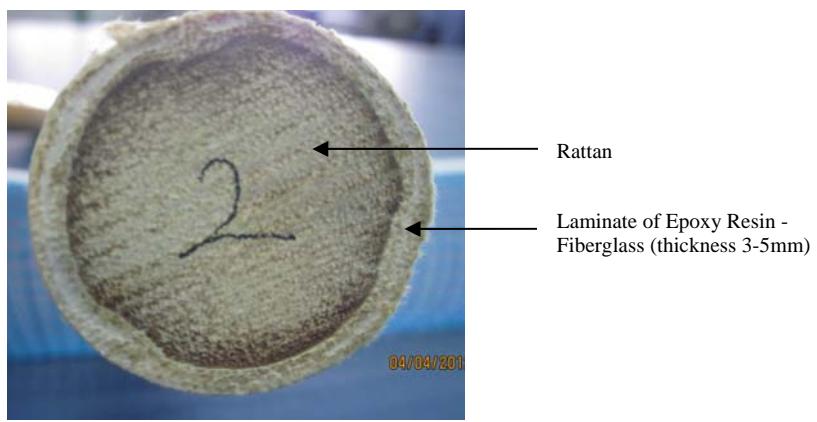


Fig. 2. Result of RLFERM manufacturing process

Tensile strength data used is the average tensile strength of 5 test samples. The results of comparison between the tensile strength and Young's Modulus of NR and RLFERM are shown in Fig. 3.

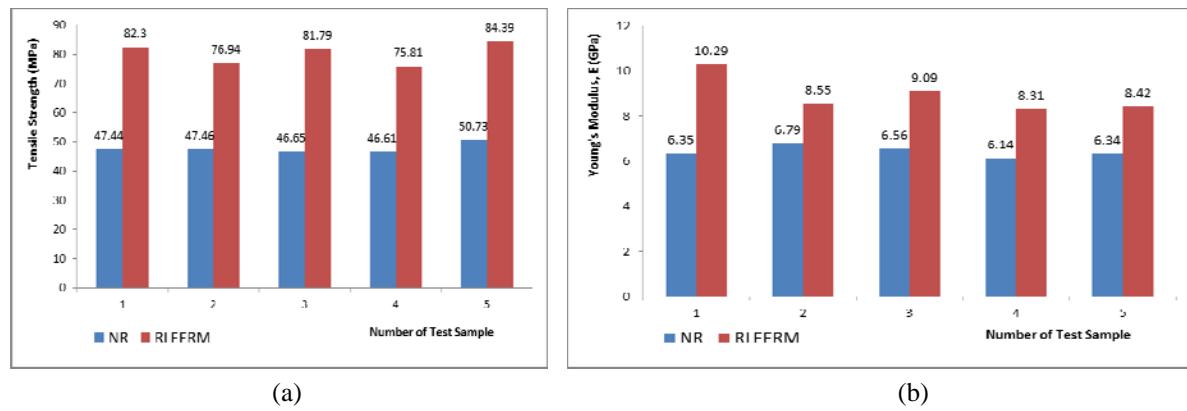


Fig. 3. Tensile strength and Young's Modulus of NR and RLFERM

Fig. 3. (a) showed that the average tensile strength of RLFERM (80.2 MPa) with Young's Modulus 8.6 GPa, increased by 67.8% when compared to the tensile strength of NR (47.8 MPa) with Young's Modulus 6.4 GPa. Based on the results of tensile strength, it can be seen that the lamination process by using epoxy resin and fiberglass is proven to increase the tensile strength. This can be obtained due to the addition of fiberglass as reinforcement rattan surface in the lamination process. The increase of tensile strength is very good and is supported by a lamination process which has been developed in this study. Lamination processes using epoxy resin reinforced with fiberglass has managed to increase the tensile strength of rattan, which is projected as a shank prosthesis endoskeletal type, as an alternative material for replacing the materials used in the design of the shank prosthesis. Tensile test results also showed an increase in Young's Modulus of RLFERM when compared to NR (Fig. 3. (b)). Enhancement of 10% is very good, so the level elasticity of RLFERM will produce a level of comfort when used by the patient, but it is still strong enough to accept the burden of the patient's weight [14]. The tensile strength test results will be a reference in the development of shank prosthesis with use of natural materials, especially rattan.

We have been calculating the tensile strength of rattan by using theoretical method and simulation by using computer software. Comparison tensile strength results of theoretical calculations and simulation by taking into account the existing cavities in rattan amounted to 0.84; the results are as follows that theoretical tensile strength: 43.9 MPa, tensile strength results of simulation by using computer software: 42.5 MPa. The difference results from theoretical calculation, simulation and testing of NR, by 8.7%. These results are quite small, so it can be used to validate the results of tensile testing of NR.

When compared with some of the results of testing the tensile strength of rattan, the strength of RLFERM is very good, because it can increase the strength of NR obtained from the free market with a low to moderate quality, becomes rattan which has high strength. Bhat *et al* [18] shows the tensile strength of rattan class I (> 70 MPa), class II (45-70 MPa) and class III (< 45 MPa). Jasni *et al* [15] shows that the value of the strength of rattan ranges between (42-83) MPa. If it is compared with this range, the tensile strength of RLFERM is included in the class I [18].



Fig. 4. Tensile Strength Sample Test of NR and RLFERM

Fig. 4 shows the difference from tensile testing result of NR and RLFERM. We can observe that NR has lower tensile strength when compared to RLFERM. It can be observed from the NR failure pattern and RLFERM due to tensile load receives. NR failure is greater than RLFERM, with a tensile load is smaller than RLFERM.

C. Compressive Strength

We have tested the compressive strength of the NR and RLFERM by using a Universal Testing Machine. Fig. 5. (b) shows that the compressive strength of the results of the simulation, theoretical calculations, and test results of NR, has acquired a very small difference. The difference is most influenced by the total surface area of

the porous surface of the rattan, which was shown in Table I. The number of pores of rattan reduces the strength generated by the rattan.

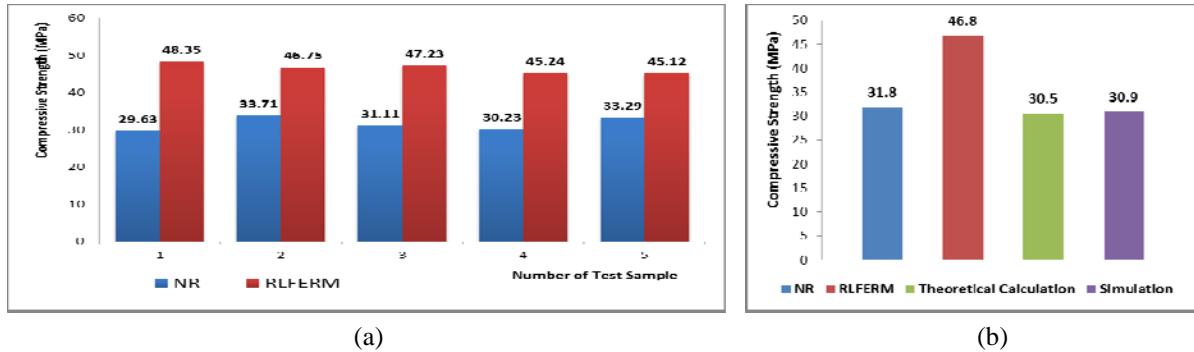


Fig. 5. Compressive Strength of NR and RLFERM

By using the theoretical reference compressive strength of 30.5 MPa, the average difference of the testing and simulation is 4.4%. The results of the compressive strength of both testing NR, the calculation of the theoretical strength and compressive strength simulation results are still in the range of research result (28.2-33.6) MPa [18], [19].

Results of the testing of compressive strength of RLFERM show an increase when compared to the compressive strength of NR (Fig. 5. (a)). With compressive strength of 46.8 MPa, it results an increase in the compressive strength of 47.2% if compare with NR (31.8 MPa). The increase in the compressive strength is greatly influenced by the surface layer of fiberglass as reinforcement rattan through the lamination process. When compared with the results of research [8], the compressive strength of rattan class I (33.6 MPa) and the compressive strength of rattan laminated epoxy resin reinforced with fiberglass, it can be obtained 39.3% greater strength. It can be concluded that the lamination process of rattan surface by using epoxy resin and reinforced with fiberglass can improve the compressive strength which is quite good when compared with NR.

D. Flexural Strength

Flexural strength is very important in the design of the prosthesis shank endoskeletal type. Good elasticity will provide a sense of comfort for the patient and the prosthesis shank is not quickly damaged due to compressive load and dynamic motion when the patient walks [1], [14]. Flexural strength is obtained from flexural testing by using a Universal Testing Machine. Fig. 6. (a) showed that flexural strength test result of RLFERM (82.3 MPa, average) is higher than the NR (54.1 MPa, average).

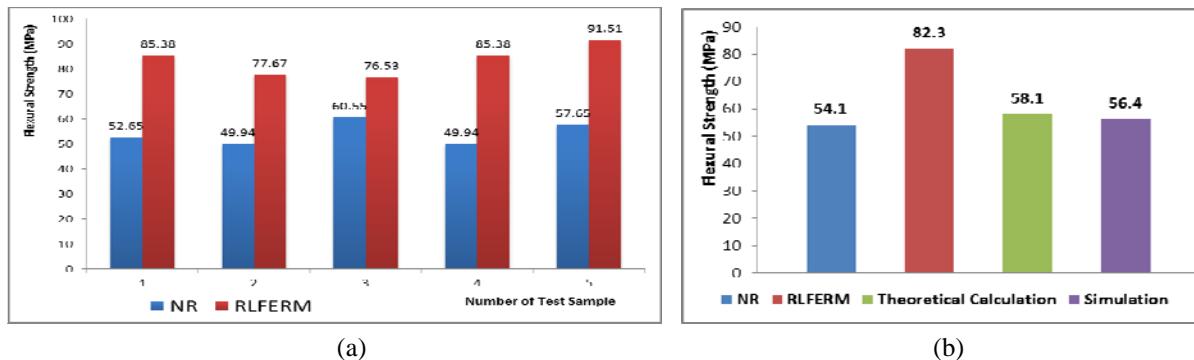


Fig. 6. Flexural strength of NR and RLFERM

The comparison of flexural strength among NR with RLFERM, theoretical calculations and simulations by using computer software are shown in Fig. 6. (b). Differences of flexural strength among NR, theoretical calculation and simulation by using computer software are 5.8% (average). These results are quite good and can be used as a reference in further development. Flexural strength of RLFERM increased on average by 52% when compared with NR. These results can be obtained because the lamination process of rattan surface by using epoxy resin and fiberglass provides a surface layer tougher and stronger. These results indicate that the epoxy resin and fiberglass lamination process has improved flexural strength of rattan.

The increase of strength of RLFERM is obtained due to the strong of bonding between the surfaces of rattan with a layer of epoxy resin reinforced with fiberglass. Good interface can occur because the rattan surface is made rough, so that fiberglass can be attached. The stockinette layer on the inner surface associated with rattan that has been made rough and the exterior parts as a binder fiberglass also increased the strength of the case.

E. Impact Strength

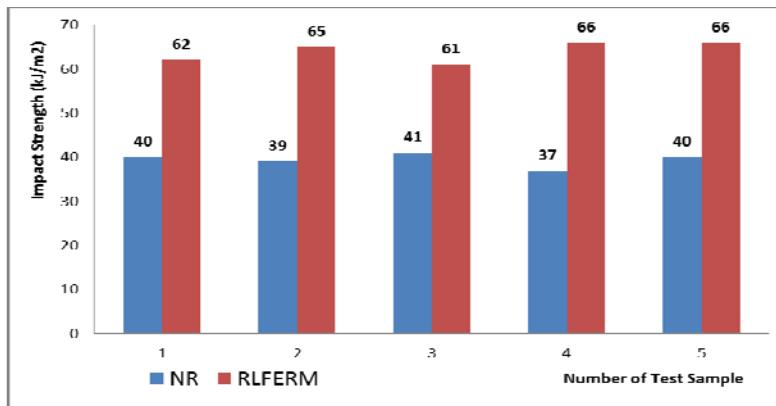


Fig. 7. Impact strength of NR and RLFERM

We have tested the strength of impact by using Charpy Impact Testing Machine. This test aims to determine the strength of rattan in receiving the impact load. Impact strength is required by the prosthesis shank material, so it can receive the load impact with other objects when used by patients [2]. The average impact strength of NR by 39 kJ/m^2 and RLFERM has increased very good by 64% to 64 kJ/m^2 (Fig. 7).

Improved impact strength is due rattan surfaces coated with an epoxy resin and fiberglass became harder and stiffer. This can be observed from the test sample which showed impact damage on the sample testing of NR is very different when compared with the results of RLFERM (Fig. 8). It can be concluded that the lamination process of rattan with epoxy resin and fiberglass, proven to improve the impact strength of rattan.

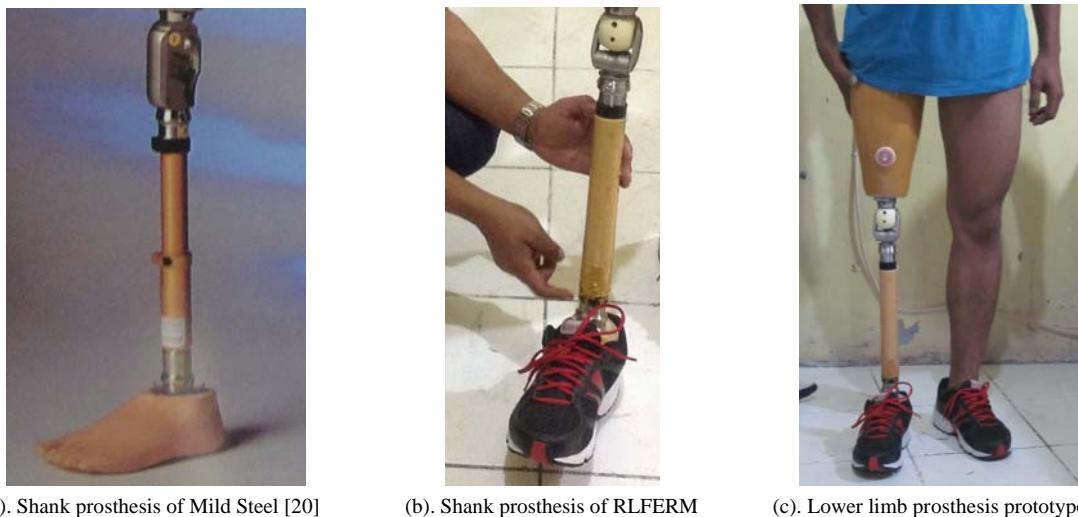


Fig. 8. Samples of compressive strength testing

F. Shank Prosthesis Prototype

To evaluate the strength of the RLFERM as an alternative material for produce shank prosthesis endoskeletal type, we have developed an initial prototype. Fig. 9. (b). shows that an initial prototype of shank prosthesis endoskeletal type made from RLFERM.

Socket, knee, shank and foot, assembled into a lower limb prosthesis as Fig. 9. (c), using a bolt connection. Bolt connection selected for ease of assembly and the replacement of components in case of damage. In general, when the prosthesis is used by the patient, the foot section will be damaged first. This happens because the part foot the main support at the time of prosthesis used to walk by the user [21]. Bolt connection will ease the process of repair or replacement in case of damage. Shank prosthesis made of RLFERM (Fig. 9. (b)), lighter than the shank prosthesis made from mild steel (Fig. 9. (a)). By using RLFERM, can be produced shank endoskeletal lighter, cheaper, Indonesia harness local potential and can be recycled. This is expected to positively impact the utilization of natural potential of Indonesia, especially rattan [10].



(a). Shank prosthesis of Mild Steel [20]

(b). Shank prosthesis of RLFERM

(c). Lower limb prosthesis prototype

Fig. 9. Shank prosthesis endoskeletal type

The first prototype of lower limb prosthesis with a shank prosthesis endoskeletal type of RLFERM, have been made with good results and tested for use by patient (Fig. 9. (c)). Shank prosthesis with RLFERM can be assembled easily to other components are socket, knee and foot. The first test results indicate that the lower limb prosthesis with a shank prosthesis components made of RLFERM can be used by patients to walk properly and has good strength. Strength and elasticity will impact on the level of safety and comfort experienced by the patient during walking using a lower limb prosthesis. It is very important to be a concern in the development of health products, especially lower limb prosthesis products [22], [23].

The results of this study can be used as a reference in the next research with increased strength and field testing process involving the patient, in order to obtain dynamic analysis to observe RLFERM strength and gait analysis when used for walking.

IV. CONCLUSION

We have developed of RLFERM as an alternative material to produce shank prosthesis endoskeletal type, by using rattan material. The use of rattan material due to the availability of abundant in Indonesia, has good strength, environmentally friendly and recyclable. The results of the macrostructure test of rattan show that solid surface area and porous parts with an average ratio of 0.84. Ratio obtained is used in the rattan strength calculation of the theoretical and simulation by using computer software. The ratio between the total surface area and pore surface area of the rattan should be taken because it affects the obtained total strength.

Manufacturing process produces a good interface between the epoxy resin, fiberglass and rattan surface. This result can be observed from the increased mechanical strength of RLFERM, including tensile strength, compressive strength, flexural strength and impact strength. The first prototype that we have developed shows that RLFERM has produced shank prosthesis endoskeletal types and can be used to walk by the patients well. The first prototype showed that patients can walk well and feel comfortable use shank prosthesis product made from RLFERM. The next study, we will observe the gait analysis and the strength of the shank prosthesis made from RLFERM when used for walking. This result will be a reference for further research in the development of a shank prosthesis made from rattan and another use in engineering design.

ACKNOWLEDGMENT

The Authors wish to thanks Research and Scientific Writing Department, Tarumanagara University for the financial support through Research University Grant.

REFERENCES

- [1] A. P. Irawan, T. P. Soemardi, K. Widjajalaksmi, and A. H. S. Reksoprodjo, "Tensile and flexural strength of ramie fiber reinforced epoxy composites for socket prosthesis application", International Journal of Mechanical and Material Engineering, vol. 6, no. 1. pp. 46-50, April 2011.
- [2] A. P. Irawan and I. W. Sukania, "Tensile and impact strength of bamboo fiber reinforced epoxy composite as alternative materials for above knee prosthesis socket", in Proc. of ICSTD, 2012, pp. M.109-M.115.
- [3] K. M. Bhat, "Grading rules for rattan a survey of existing rules and proposal for standardization", International Network for Bamboo and Rattan, 1996.
- [4] S. Patterson, "Advancing orthotic and prosthetic care through knowledge", The Academic Today, vol. 3, No. 3, June 2007.
- [5] G. Stark, "Perspectives on how and why feet are prescribed", Journal of Prosthetics and Orthotics, vol. 17, Num. 4S, pp. 18- 22, 2005.
- [6] J. A. Campbell, "Material selection in an above knee prosthetic leg", Engineering Materials, Department of Engineering, Australian National University, 2002.
- [7] V. Faulkner, M. Field, J. W. Egan, and N. G. Gall, "Evaluation of high strength materials for prostheses", Orthotics and Prosthetics, vol. 40, no. 4, pp. 44-58, 1987.

- [8] K. A. Khazraji, J. Kadhim, and P. S. Ahmed, "Tensile and fatigue characteristics of lower-limb prosthetic socket made from composite materials", in Proc. of the 2012 International Conference on Industrial Engineering and Operations Management Istanbul, Turkey, pp. 843-852, July 2012.
- [9] J. Craig, "Prosthetic feet for low-income countries", Journal of Prosthetics and Orthotics, vol. 17, Num. 4S, pp. 27- 49, 2005.
- [10] A. P. Irawan and I. W. Sukania, "Mechanical characteristics rattan fiber reinforced epoxy composites (RECO) as above knee socket prosthesis materials", in Proc. of IPST, 2011, pp. 64-70.
- [11] A. P. Irawan and I. W. Sukania, "Tensile Strength of banana fiber reinforced epoxy composites materials", Applied Mechanics and Materials, vol. 776, 2015, pp. 260-263.
- [12] H. N. Shasmin, N. A. A. Osman, and A. A. Latif, "Economical tube adapter material in below knee prosthesis", in Proc. Biomed, 2008, pp. 407- 409.
- [13] K. Muniandy, H. Ismail, and N. Othman, "Curing characteristics and mechanical properties of rattan filled natural rubber compounds", Key Engineering Materials, vol. 471-472, pp. 845-850, 2011.
- [14] A. P. Irawan, T. P. Soemardi, W. Kusumaningsih, A. H. S. Reksoprodjo, "Gait analysis of the prosthesis prototype made from the natural fiber reinforced composite", in Proc. APCHI-ERGOFUTURE 2010, 2010, pp. 37-43, Aug 2010.
- [15] Jasni, D. Martono, and N. Supriana, "Sari hasil penelitian rotan", Buletin Dephut, 2007.
- [16] Krisdianto and Jasni, "Struktur anatomi tiga jenis batang rotan, Jurnal Ilmu & Teknologi Kayu Tropis, vol. 3, no. 2, 2005.
- [17] A.T. Tellu, Kladistik, "Beberapa jenis rotan calamus spp. Asal sulawesi tengah berdasarkan karakter fisik dan mekanik batang", Jurnal Biodiversitas, vol. 7, no. 3, pp. 225-22, July 2006.
- [18] K. M. Bhat and P. K. Thulasidas, "Strength properties of ten South Indian canes", Journal of Tropical Forest Science, vol 5, no. 1, pp. 26-34, 1992.
- [19] D. Sebayang, T. I. King, and R. B. Wahab, "The properties of rattan calamus caesius (rattan saga) and its application in spring form", Indonesian Journal of Materials Science, vol. 5, no. 2, pp. 21-26, June 2004.
- [20] Otto Bock, "Prosthetics lower extremities, technology for people", Anniversary Edition, 2009.
- [21] C. C. L. Winson, M. Zhang, D. A. Boone, and B. Contoyannis, "Finite-element analysis to determine effect of monolimb flexibility on structural strength and interaction between residual limb and prosthetic socket", Journal of Rehabilitation Research and Development, vol. 41, no. 6A, pp. 775-796, November/December 2004.
- [22] R. L. Braddom, Physical Medicine & Rehabilitation, Second Edition, W. B. Saunders Company, Philadelphia, 2000.
- [23] A. P. Irawan, F. Fediyanto, and S. Tandi, "The design of bicycle for disable with ergonomic aspect consideration", in Proc. Ergo Future 2006, pp. 337-341, Aug 2016.
- [24] M. S. Sander and M.C. J. Ernest, Human Dimension and In Engineering and Design, 7th Editions , McGraw-Hill Inc Singapore, 1992.

Document details

1 of 1

[CSV export](#)  [Download](#)  [Print](#)  [E-mail](#)  [Save to PDF](#)  [Save to list](#) [More...](#)

International Journal of Engineering and Technology
Volume 8, Issue 3, 1 July 2016, Pages 1543-1550

Mechanical characteristics of rattan reinforced fiberglass and epoxy composites for shank prosthesis application (Article)

Irawan, A.P. , Daywin, F.J., Fanando, Agustino, T. 

 [Save all to author list](#)

Faculty of Engineering, Mechanical Engineering Department, Tarumanagara University, Jl. Letjen. S. Parman No. 1, Jakarta, 11440, Indonesia

Abstract

 [View references \(24\)](#)

This research aims to develop a rattan laminated fiberglass epoxy resin materials (RLFERM) to increase of mechanical strength especially in tensile, compressive, impact and flexural strength. The RLFERM will be used as an alternative material for shank prosthesis endoskeletal type and another use in engineering design. This research is related to the utilization of the natural potential of Indonesia especially of rattan. The method used to produce the endoskeletal material by using laminated process of rattan with fiberglass and epoxy resin. The test conducted involves the tensile, compressive, impact and flexural strength. The result showed that there was an increase in strength of RLFERM compared with rattan without lamination (Natural Rattan, NR). Tensile strength of RLFERM (80.2 MPa) and E = 8.6 GPa increased by 67.8% when compared to the tensile strength of NR (47.8 MPa) and E = 6.4 GPa. Compressive strength of RLFERM increased 47.2%, from 31.8 MPa to 46.8 MPa, impact strength of RLFERM increased 64%, from 39 kJ/m² to 64 kJ/m², and flexural strength of RLFERM increased on average by 53% from 54.1 MPa to 82.3 MPa. Increasing strength of RLFERM is obtained from good interface between surface of rattan with fiberglass and epoxy resin as laminate. The first prototype of lower limb prosthesis with a shank prosthesis endoskeletal type of RLFERM, have been made with good results and tested for use by patient. The test results indicate that the lower limb prosthesis with a shank prosthesis components made from RLFERM can be used by patients to walk properly and has good strength. This result will be a reference for further research in the development of a shank prosthesis made from rattan and another use in engineering design.

SciVal Topic Prominence

Topic: Prostheses | Amputation | Liner

Prominence percentile: 87.241 

Author keywords

[Endoskeletal type](#) [Laminated](#) [Mechanical strength](#) [Rattan](#) [Shank](#)

ISSN: 23198613

Source Type: Journal

Original language: English

Document Type: Article

Publisher: Engg Journals Publications

References (24)

[View in search results format](#) 

All [CSV export](#)  [Download](#)  [Print](#)  [E-mail](#)  [Save to PDF](#) [Create bibliography](#)

1 Irawan, A.P., Soemardi, T.P., Widjajalaksmi, K., Reksoprodjo, A.H.S. **Tensile and flexural strength of ramie fiber reinforced epoxy composites for socket prosthesis application** (2011) *International Journal of Mechanical and Materials Engineering*, 6 (1), pp. 46-50. Cited 28 times.

Metrics  [View all metrics](#) 

13 Citations in Scopus

70th percentile

0.96 Field-Weighted Citation Impact 



PlumX Metrics

Usage, Captures, Mentions, Social Media and Citations beyond Scopus.

Cited by 13 documents

Utilization of machining technology in the production process of Jepara wood carving furniture

Supriyatna, E., Irawan, A.P., Maitri Widya, M. (2020) *IOP Conference Series: Materials Science and Engineering*

Design of prosthesis by sustainable aluminium 2024-t4 material under various load conditions using tetrahedral mesh

Sankaran, S., Pallikonda Rajasekaran, M. (2020) *Journal of Green Engineering*

Development of wood carving furniture technology in Jepara

Marizar, E.S., Mutiara, M.W., Irawan, A.P. (2020) *IOP Conference Series: Materials Science and Engineering*

[View all 13 citing documents](#)

Inform me when this document is cited in Scopus:

[Set citation alert](#) 

Related documents

Gait analysis of the prosthesis prototype made from the natural fiber reinforced composite



Source details

International Journal of Engineering and Technology

CiteScore 2015
0.8 [ⓘ](#)

Scopus coverage years: from 2009 to 2017

(coverage discontinued in Scopus)

Publisher: Engg Journals Publications

SJR 2019
0.103 [ⓘ](#)

ISSN: 2319-8613 E-ISSN: 0975-4024

Subject area: [Engineering: General Engineering](#)

Source type: Journal

SNIP 2019
0.504 [ⓘ](#)[View all documents >](#)[Set document alert](#)[Save to source list](#)[CiteScore](#) [CiteScore rank & trend](#) [Scopus content coverage](#)

i Improved CiteScore methodology

CiteScore 2015 counts the citations received in 2012-2015 to articles, reviews, conference papers, book chapters and data papers published in 2012-2015, and divides this by the number of publications published in 2012-2015. [Learn more >](#)

CiteScore 2015

0.8 = $\frac{978 \text{ Citations 2012 - 2015}}{1,201 \text{ Documents 2012 - 2015}}$

Calculated on 01 May, 2016

 [ⓘ](#)

= —

CiteScore rank 2015 [ⓘ](#)

Category	Rank	Percentile
----------	------	------------

Engineering
General
Engineering

#145/273 47th

[View CiteScore methodology >](#) [CiteScore FAQ >](#) [Add CiteScore to your site ↗](#)

About Scopus

[What is Scopus](#)
[Content coverage](#)
[Scopus blog](#)
[Scopus API](#)
[Privacy matters](#)

Language

[日本語に切り替える](#)
[切换到简体中文](#)
[切换到繁體中文](#)
[Русский язык](#)

Customer Service

[Help](#)
[Contact us](#)

ELSEVIER[Terms and conditions ↗](#) [Privacy policy ↗](#)

Copyright © Elsevier B.V. All rights reserved. Scopus® is a registered trademark of Elsevier B.V.

We use cookies to help provide and enhance our service and tailor content. By continuing, you agree to the use of cookies.



This author profile is generated by Scopus [Learn more](#)

Irawan, Agustinus Purna

[i](#) Tarumanagara University, Jakarta, Indonesia [Show all author info](#)

[SC](#) 37124009300 [i](#) [ID](#) <https://orcid.org/0000-0002-9055-2014>

[✉](#) Is this you? Connect to Mendeley account

[Edit profile](#) [Set alert](#) [Save to list](#) [Potential author matches](#)
[Export to SciVal](#)


Metrics overview

37 Documents by author

79 Citations by 54 documents

5 h-index: [View h-graph](#)

Document & citation trends

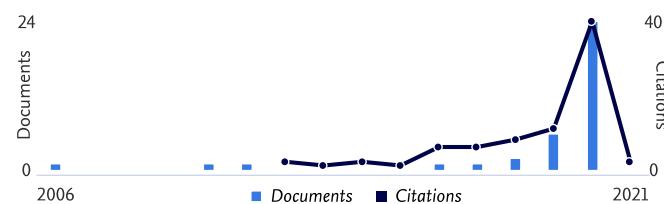

[Analyze author output](#) [Citation overview](#)

Most contributed Topics 2015–2019 [i](#)

Prostheses; Amputation; Liner

3 documents

Kenaf Fibers; Sisal; Coir

1 document

Spur Gears; Rattle; Fused Teeth

1 document

[View all Topics](#)

37 Documents Cited by 54 Documents 0 Preprints 81 Co-Authors [Topics](#)

[Export all](#) [Save all to list](#)

Sort by: [Cited by \(highest\)](#) [▼](#)

[View list in search results format](#)

Article

Tensile and flexural strength of ramie fiber reinforced epoxy composites for socket prosthesis application

28

Cited by

[View references](#)

Irawan, A.P., Soemardi, T.P., Widjajalaksmi, K., Reksoprodjo, A.H.S.

International Journal of Mechanical and Materials Engineering, 2011, 6(1), pp. 46–50

[View abstract](#) [▼](#) [Related documents](#) [DOC XML](#) [SOLR JSON](#)

Article

Mechanical characteristics of rattan reinforced fiberglass and epoxy composites for shank prosthesis application

13

Cited by

Irawan, A.P., Daywin, F.J., Fanando, Agustino, T.

International Journal of Engineering and Technology, 2016, 8(3), pp. 1543–1550

[View abstract](#) [▼](#) [Related documents](#) [DOC XML](#) [SOLR JSON](#)

International Journal of Engineering and Technology

Discontinued in Scopus as of 2017

COUNTRY	SUBJECT AREA AND CATEGORY	PUBLISHER	H-INDEX
India  Universities and research institutions in India	Chemical Engineering Fluid Flow and Transfer Processes Engineering Aerospace Engineering Mechanical Engineering	Engg Journals Publications	24

PUBLICATION TYPE	ISSN	COVERAGE
Journals	23198613, 09754024	2009-2018

SCOPE

Information not localized

 Join the conversation about this journal

 Quartiles
